

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWF-0382
Location:	WEST WINDSOR POLICE	
Calibration File No.:	01604	Calib. Date: 07/29/2019
Certification File No.:	01605	Cert. No.: 00046
Linearity File No.:	01606	Cert. Date: 07/29/2019
Solution File No.:	01608	Lin. Date: 07/29/2019
Sequential File No.:	01608	Lin. No.: 00032
		Soln. Date: 08/27/2019
		Soln. No.: 00254
		File Date: 08/27/2019
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWJ S3-0364
Solution Control Lot:	18320	Expires: 09/26/2020
		Bottle No.: 0104

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:16D		
Control 1 EC	0.100%	11:17D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	11:17D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:17D		
Control 2 EC	0.099%	11:18D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	11:18D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:19D		
Control 3 EC	0.100%	11:19D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	11:19D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:20D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: BAL

First Name: FRANK

MI: N

Signature: _____

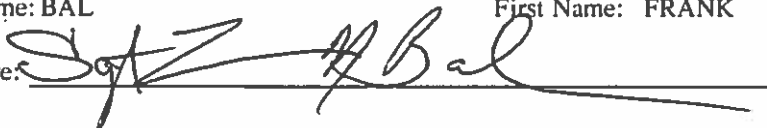

Badge No.: 467

Date: 08/27/2019