

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWF-0382
Location:	WEST WINDSOR POLICE	
Calibration File No.:	01445	Calib. Date: 07/26/2017
Certification File No.:	01446	Calib. No.: 00041
Linearity File No.:	01447	Cert. Date: 07/26/2017
Solution File No.:	01454	Cert. No.: 00028
Sequential File No.:	01454	Lin. Date: 07/26/2017
		Lin. No.: 00027
		Soln. Date: 09/18/2017
		Soln. No.: 00219
		File Date: 09/18/2017
Calibrating Unit:	4	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWJ S3-0364
Solution Control Lot:	16330	Expires: 10/28/2018
		Bottle No.: 0581

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:32D		
Control 1 EC	0.100%	12:33D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	12:33D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:34D		
Control 2 EC	0.101%	12:34D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	12:34D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:35D		
Control 3 EC	0.101%	12:35D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	12:35D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:36D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: LATORRE

First Name: FRANCESCO

MI: -

Signature: _____

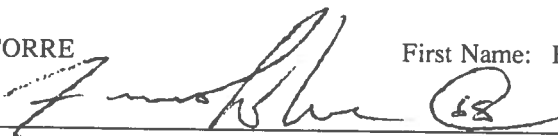

Badge No.: 68

Date: 09/18/2017